


👯 eurofins

Eurofins Water Hygiene Testing UK Sample Volume Guide

Example sample bottle

Required fill volume to 1000ml line Insufficient sample in this bottle as it is below the fill line

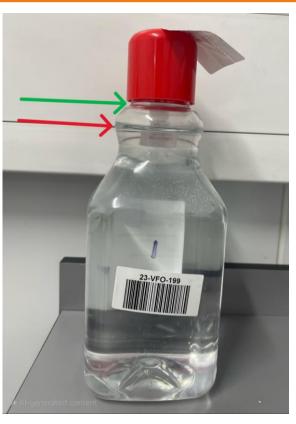

Legionella sample volume requirements

As part of our UKAS No. 9658 accreditation, it is important that a sufficient sample volume for *Legionella* analysis is submitted to the laboratory. This helps us ensure that results are accurate, reliable, and fully within the scope of our accreditation.

Requirements for submission

- Each bottle should be filled to on or above the 1000ml line, clearly marked at the base of the neck
- Where less than 1000ml is received, we will filter 500ml (where possible) and report results based on this volume
- Bottle caps must be tightly secured to avoid leakage during transport

We kindly ask for your continued cooperation in filling bottles to the required volume and securing caps firmly before collection.